


Your chair is ready for use.

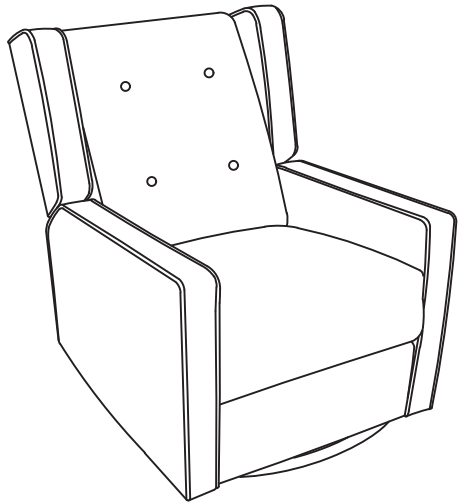

CARE INSTRUCTIONS:

WIPE CLEAN WITH A SOFT DAMP OR DRY CLOTH. DO NOT USE ABRASIVE MATERIALS AND SOLVENTS. CHECK AND TIGHTEN ALL PARTS REGULARLY. KEEP AWAY FROM WATER AND DIRECT SUNLIGHT. STORE IN A DRY PLACE. FOR INDOOR AND DOMESTIC USE ONLY.

WARNING:

DO NOT STAND ON THIS CHAIR. DO NOT USE THIS CHAIR AS A STEP LADDER. DO NOT SIT ON THE ARMRESTS OF CHAIR. SUITABLE FOR ONE PERSON ONLY. ONLY USE ON A FLAT SURFACE. FAILURE TO FOLLOW THESE WARNINGS COULD RESULT IN SERIOUS INJURY. THIS PACKAGING CONTAINS SMALL PARTS AND SHARP POINTS. KEEP UNASSEMBLED PARTS AWAY FROM CHILDREN AND BABIES.

MAXIMUM LOAD WEIGHT: 100KGS

Drawings in the manual are for visual purposes only. Actual product may vary slightly.

Adult assembly required.

KEYCODE: 43-068-487

MADE IN CHINA

FOR AU / NZ: IMPORTED FOR KMART STORES IN AUSTRALIA AND NEW ZEALAND.

KMART CUSTOMER SERVICE


AU: 1800 124 125 NZ: 0800 945 995

anko

Nursing Glider Chair Installation Manual





100
kg

MAXIMUM
LOAD WEIGHT

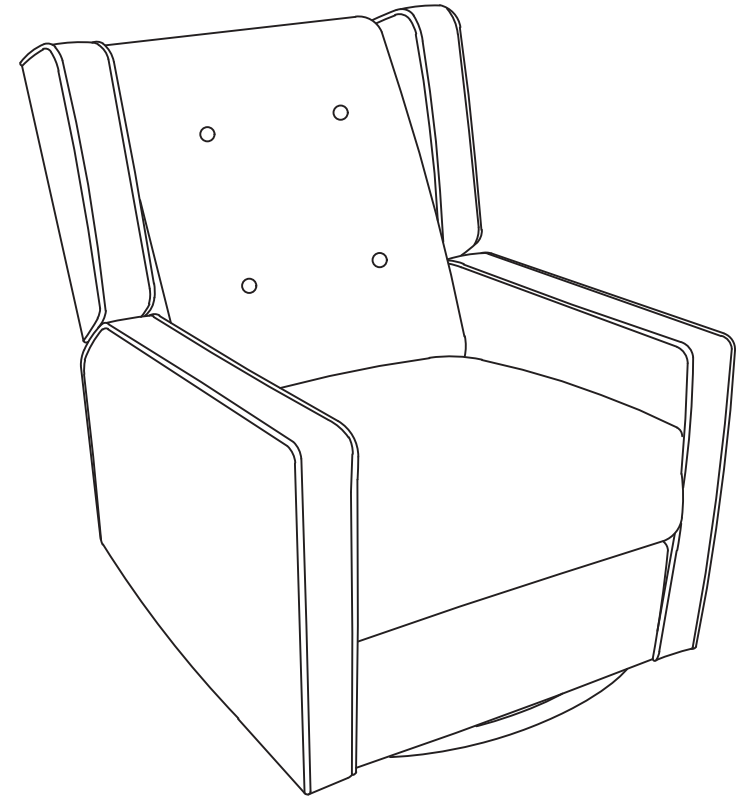


THE ILLUSTRATIONS SHOWN IN THIS MANUAL ARE FOR REFERENCE ONLY. THE MANUFACTURER RESERVES THE RIGHT TO CHANGE ANY SPECIFICATION OR FEATURE WITHOUT FURTHER NOTICE. PLEASE READ CAREFULLY BEFORE USE AND KEEP FOR FUTURE REFERENCE.

Parts List
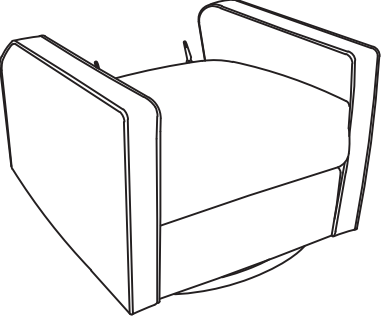
| | |
|--|--|
| <p>AX1</p>  | <p>BX1</p>  |
| <p>CX1</p>  | <p>DX1</p>  |


Assembly

Step 1: Affix parts C & D with part B.

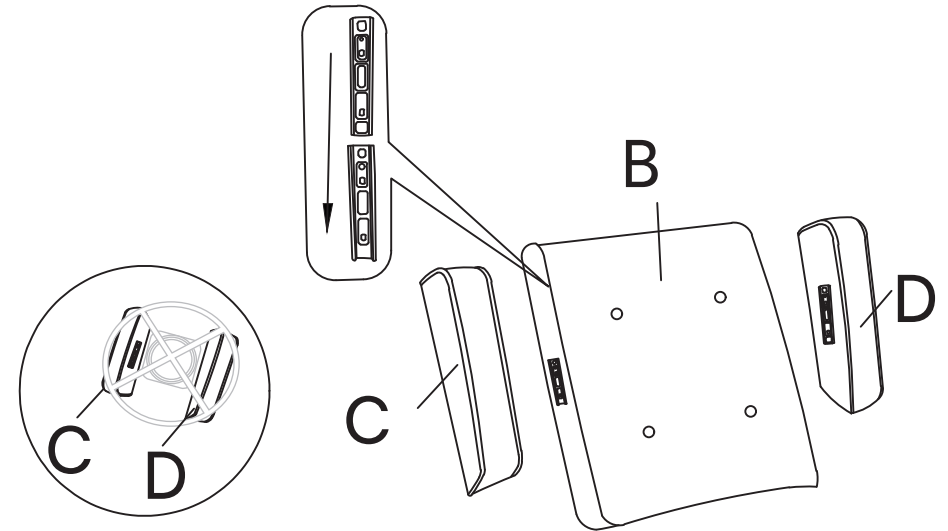

Tips: Please untie the rope, then take put part C and D from base.

Step 2: Affix parts C, B & D with part A.

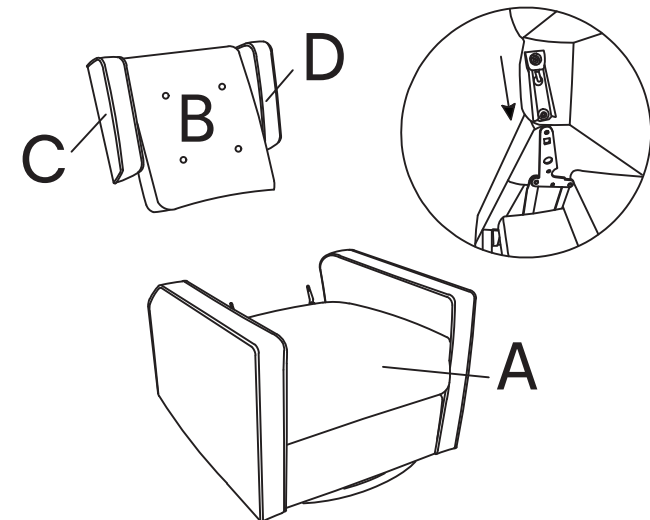

Note: please pay attention to remove the protective cover of the bottom steel frame.